


Supplementary Material

Supplementary Figure 1: Consensus agreement scores by number of years of experience with implanting cardiac pacing devices. Note: the dark green line represents consensus threshold of 66% and the light green line represents the threshold for very high consensus (90%)



Supplementary Figure 2: Consensus agreement scores by number of years of experience with implanting leadless cardiac pacing devices. Note: the dark green line represents consensus threshold of 66% and the light green line represents the threshold for very high consensus (90%)

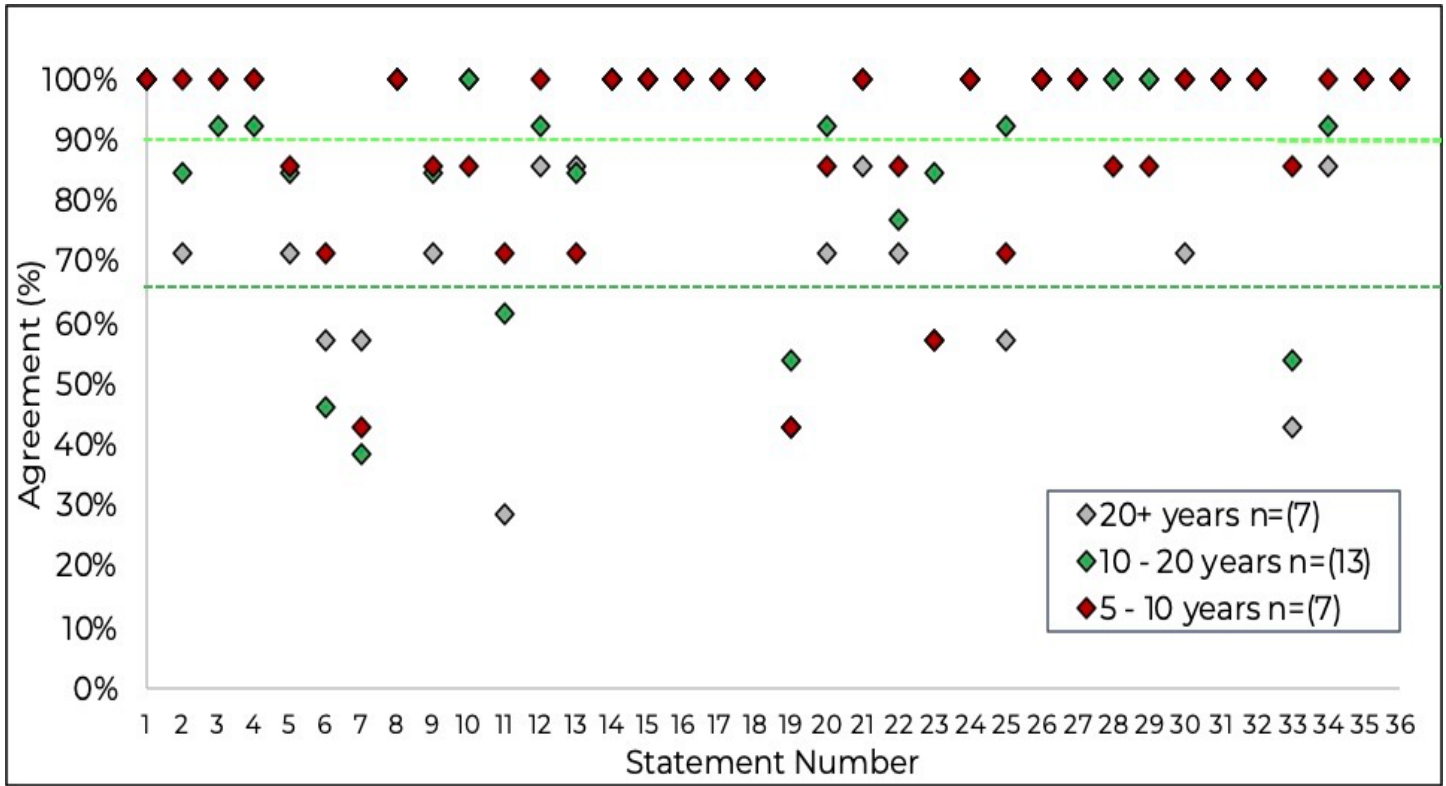